



USSN 10/525,227 – Hiroshi KOH
 Harmonic Diagnosing Method for Electric Facility
 Attorney Docket 58544.1500
 REPLACEMENT SHEET

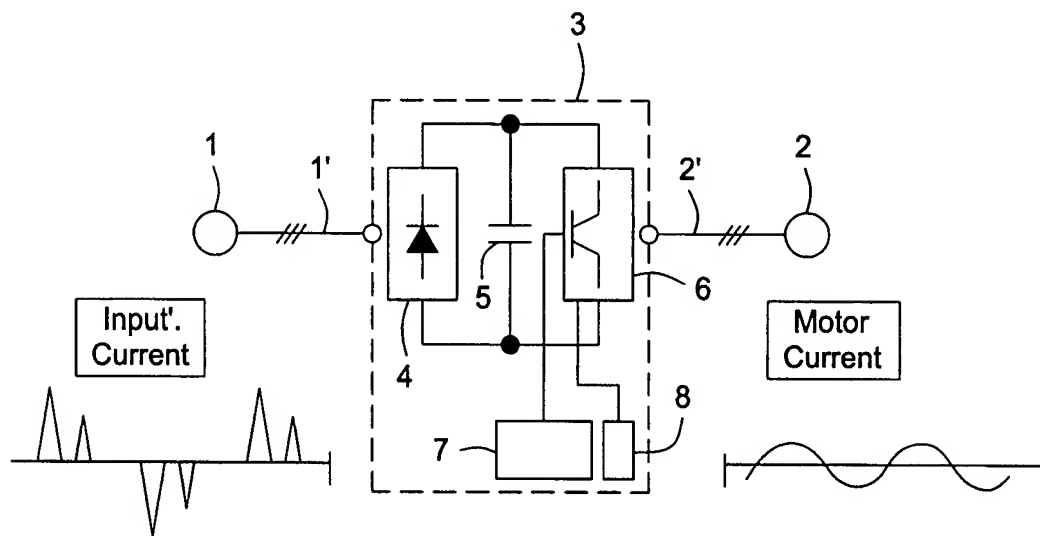


FIG. 1
 (PRIOR ART)

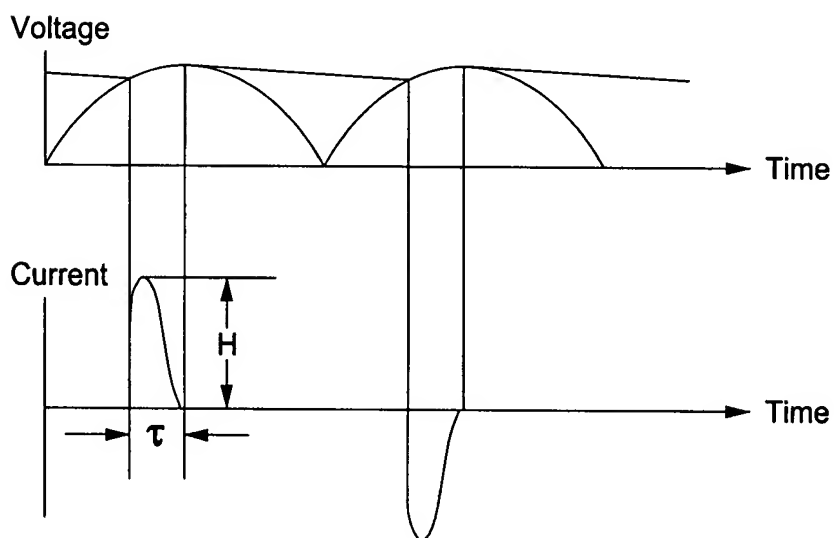


FIG. 2
 (PRIOR ART)



USSN 10/525,227 – Hiroshi KOH
Harmonic Diagnosing Method for Electric Facility
Attorney Docket 58544.1500
REPLACEMENT SHEET

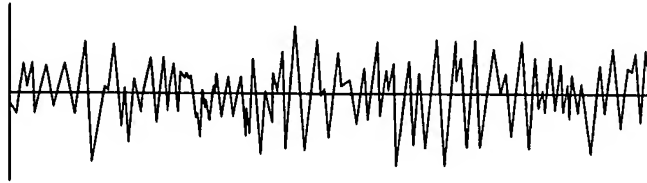


FIG. 3A

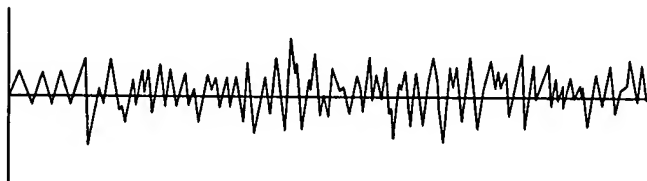


FIG. 3B



FIG. 3C



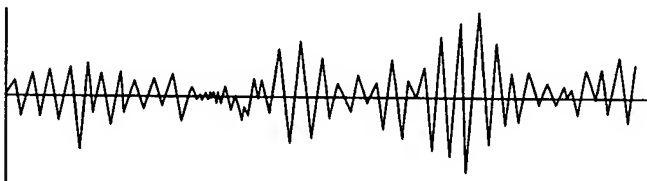


FIG. 3D

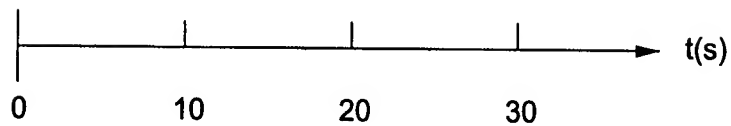

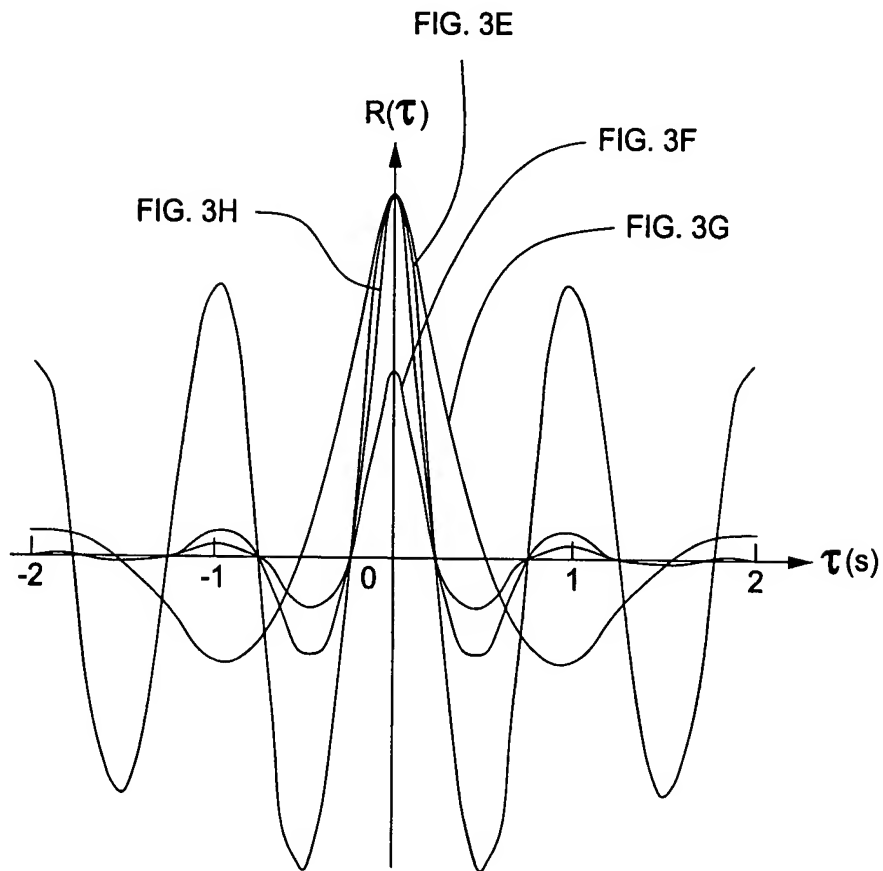

USSN 10/525,227 – Hiroshi KOH
Harmonic Diagnosing Method for Electric Facility
Attorney Docket 58544.1500
REPLACEMENT SHEET



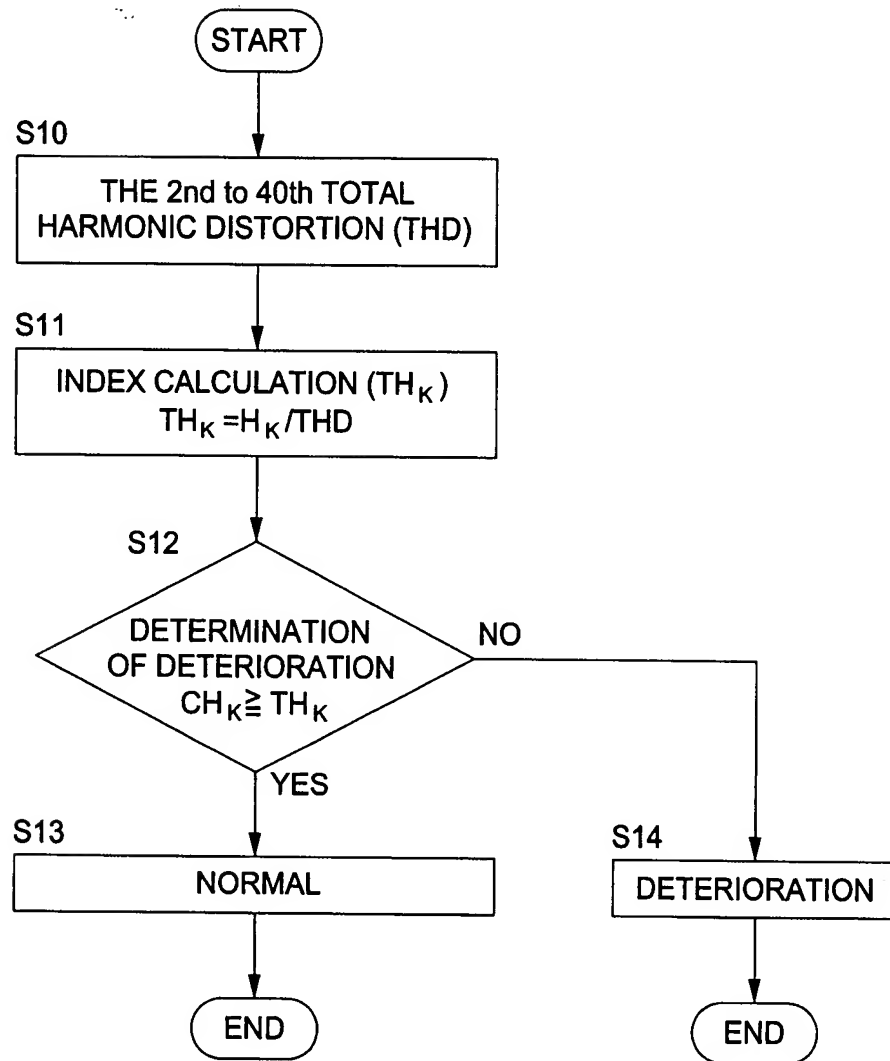


FIG. 4

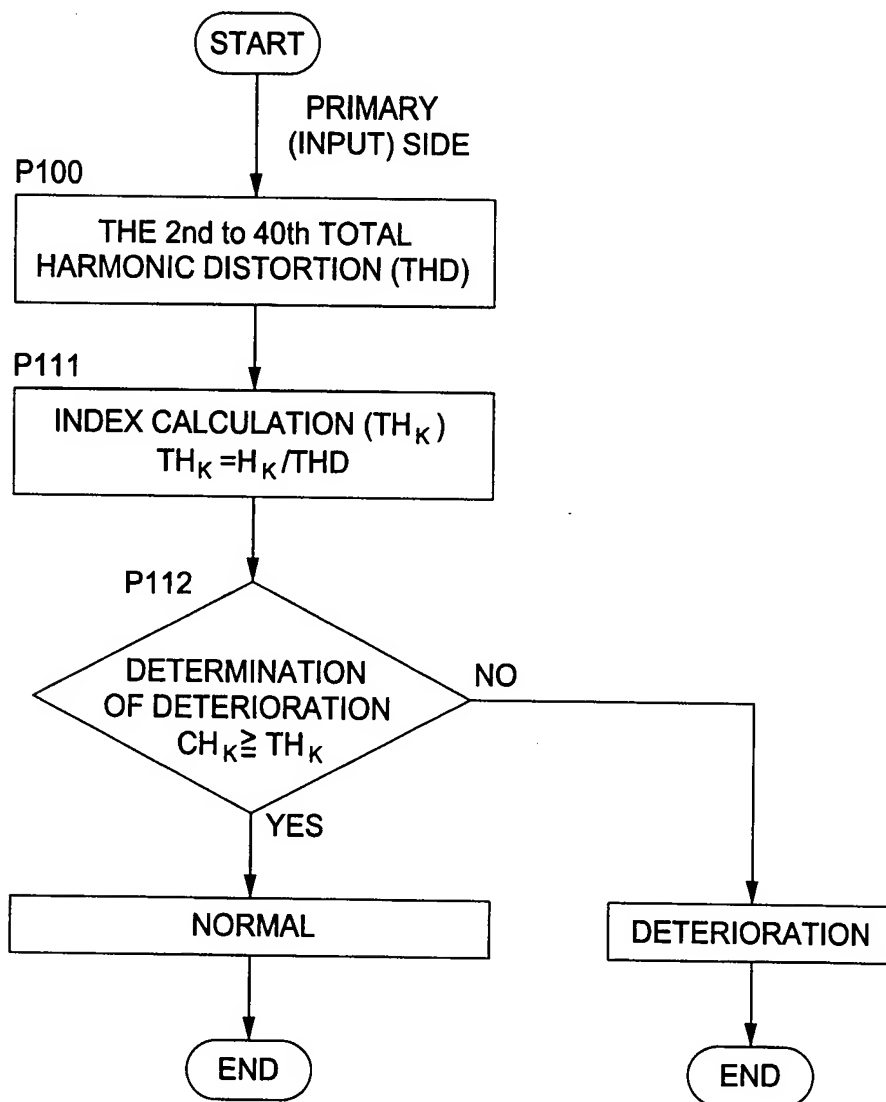


FIG. 5A

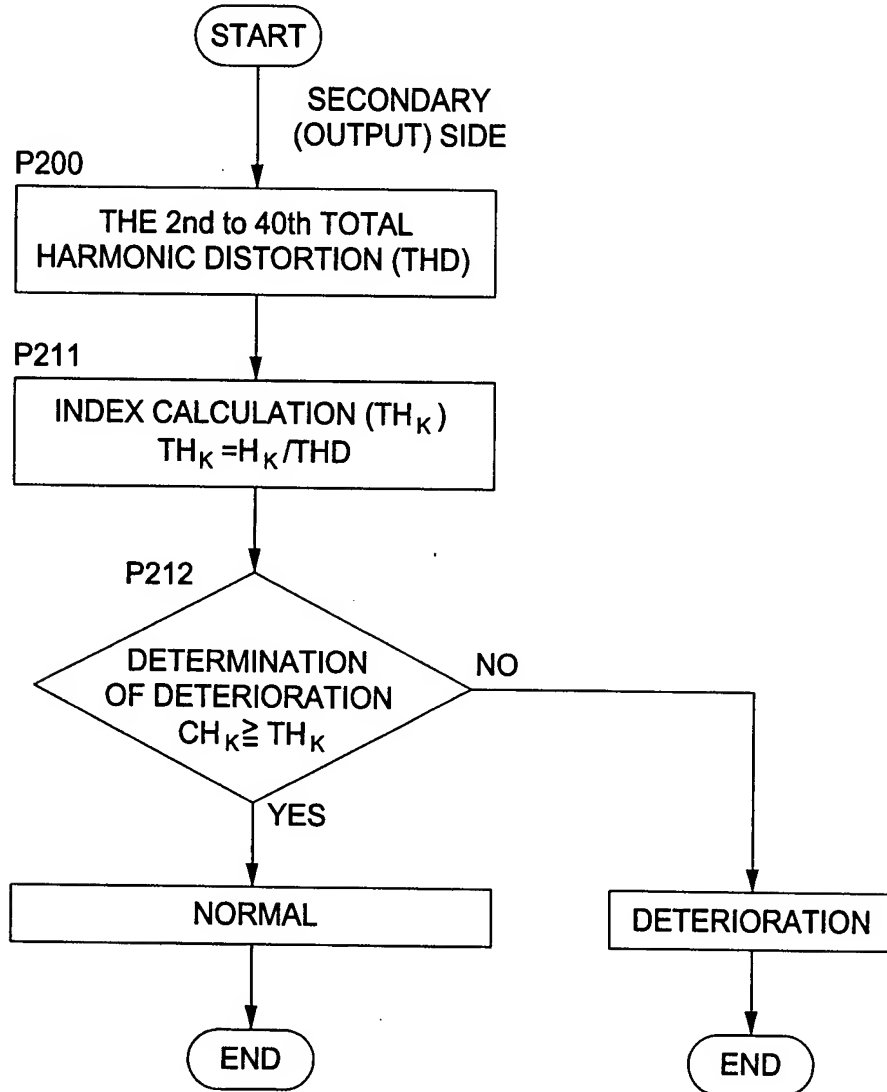


FIG. 5B

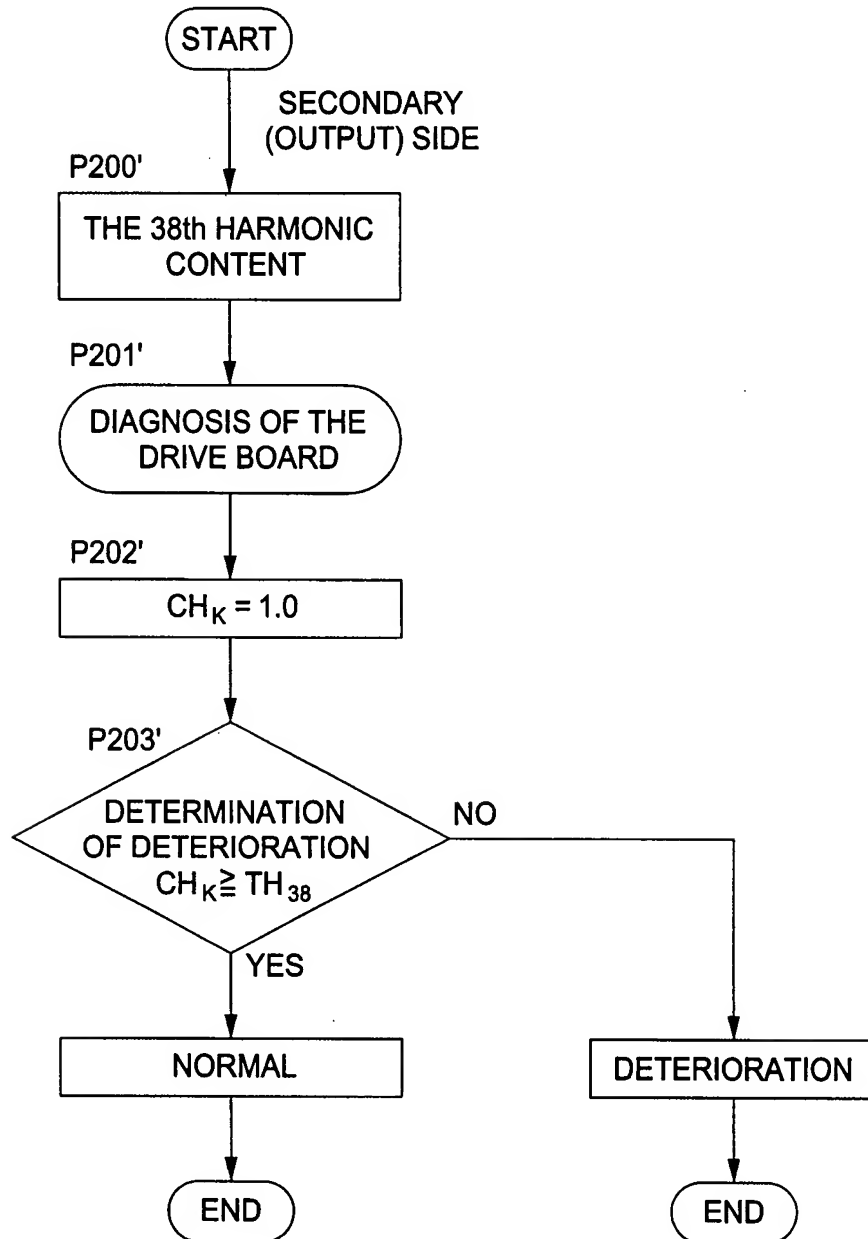


FIG. 5C